

# Appendix C

---

Calibration Certificate for  
Construction Dust Monitoring  
Equipment



**TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET**

Location : M-A3	Date of Calibration: 11-May-20
Location : S.K.H Tsoi Kung Po Secondary School	Next Calibration Date: 10-Aug-20
Make: <input type="text" value="Tisch"/>	Technician: Felix Fong
Model: <input type="text" value="TE-5170"/>	S/N: <input type="text" value="4388"/>

CONDITIONS			
Sea Level Pressure (hPa):	1010.3	Corrected Pressure (mm Hg):	758
Temperature (°C):	28.9	Temperature (K):	292

CALIBRATION ORIFICE			
Make:	<input type="text" value="Tisch"/>	Qstd Slope:	<input type="text" value="2.08799"/>
Model:	<input type="text" value="TE-5025A"/>	Qstd Intercept:	<input type="text" value="-0.03545"/>
Calibration Date:	<input type="text" value="21-Oct-19"/>	Expiry Date:	<input type="text" value="21-Oct-20"/>
S/N:	<input type="text" value="2456"/>		

CALIBRATIONS							
Plate No.	H2O (L) (in)	H2O (R) (in)	H2O (in)	Qstd (m <sup>3</sup> /min)	I (chart)	IC (corrected)	LINEAR REGRESSION
18	4.00	-8.60	12.600	1.732	56.00	56.50	Slope = 54.4569 Intercept = -36.4615 Corr. coeff.= 0.9905
13	3.60	-7.50	11.100	1.627	52.00	52.46	
10	3.00	-6.80	9.800	1.530	48.00	48.43	
7	2.20	-6.40	8.600	1.434	42.00	42.38	
5	1.30	-5.60	6.900	1.286	32.00	32.29	


**Calculations:**

Qstd = 1/m[√(H2O(Pa/Pstd)(Tstd/Ta))-b]  
IC = I[√(Pa/Pstd)(Tstd/Ta)]

- Qstd = standard flow rate
- IC = corrected chart response
- I = actual chart response
- m = calibrator Qstd slope
- b = calibrator Qstd intercept
- Ta = actual temperature during calibration (deg C)
- Pa = actual pressure during calibration (mm Hg)
- Tstd = 298 deg K
- Pstd = 760 mm Hg

**For subsequent calculation of sampler flow**  
1/m((I[√(298/Tav)(Pav/760)]-b)

- m = sampler slope
- b = sampler intercept
- I = chart response
- Tav = daily average temperature
- Pav = daily average pressure

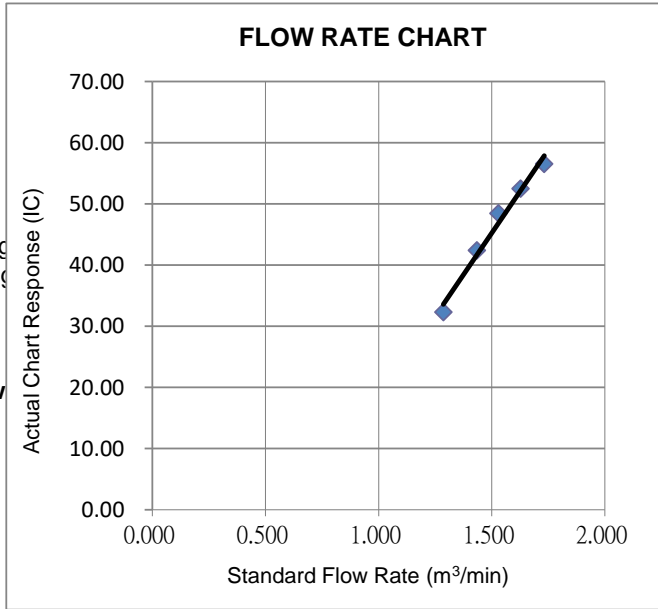

# Certificate of Calibration

Calibration Certification Information			
Cal. Date: October 21, 2019	Rootsmeter S/N: 438320	Ta: 295	°K
Operator: Jim Tisch		Pa: 744.2	mm Hg
Calibration Model #: TE-5025A	Calibrator S/N: <b>2456</b>		

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.4200	3.2	2.00
2	3	4	1	1.0180	6.3	4.00
3	5	6	1	0.9030	7.9	5.00
4	7	8	1	0.8620	8.8	5.50
5	9	10	1	0.7120	12.6	8.00

Data Tabulation						
Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left( Ta/Pa \right)}$ (y-axis)	
0.9849	0.6936	1.4066	0.9957	0.7012	0.8904	
0.9808	0.9635	1.9892	0.9915	0.9740	1.2592	
0.9787	1.0838	2.2240	0.9894	1.0957	1.4078	
0.9775	1.1340	2.3325	0.9882	1.1464	1.4765	
0.9724	1.3658	2.8131	0.9831	1.3807	1.7808	
<b>QSTD</b>	<b>m=</b>	<b>2.08799</b>	<b>QA</b>	<b>m=</b>	<b>1.30746</b>	
	<b>b=</b>	<b>-0.03545</b>		<b>b=</b>	<b>-0.02244</b>	
	<b>r=</b>	<b>0.99989</b>		<b>r=</b>	<b>0.99989</b>	

Calculations			
Vstd=	$\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va=	$\Delta Vol((Pa-\Delta P)/Pa)$
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime
For subsequent flow rate calculations:			
Qstd=	$1/m \left( \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left( \left( \sqrt{\Delta H \left( Ta/Pa \right)} \right) - b \right)$

Standard Conditions	
Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH: calibrator manometer reading (in H2O)	
ΔP: rootsmeter manometer reading (mm Hg)	
Ta: actual absolute temperature (°K)	
Pa: actual barometric pressure (mm Hg)	
b: intercept	
m: slope	

RECALIBRATION
US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30

## CALIBRATION CERTIFICATE

Date: August 28th, 2019

Equipment Name	:	Digital Dust Indicator, Model LD-5R
Code No.	:	080000-72
Quantity	:	1 unit
Serial No.	:	882148
Sensitivity	:	0.001 mg/m <sup>3</sup>
Sensitivity Adjustment	:	618
Scale Setting	:	August 23rd, 2019

We hereby certify that the above mentioned instrument has been calibrated satisfactory.

Sincerely

**SIBATA SCIENTIFIC TECHNOLOGY LTD.**

*Tong Zhang*

Tong Zhang  
Overseas & New Business Group  
Overseas Sales Department

